


Best Available Copy

Best Available Copy

FIG. 2

From Asian Cardiovasc Thorac Ann 1999;7:349-352

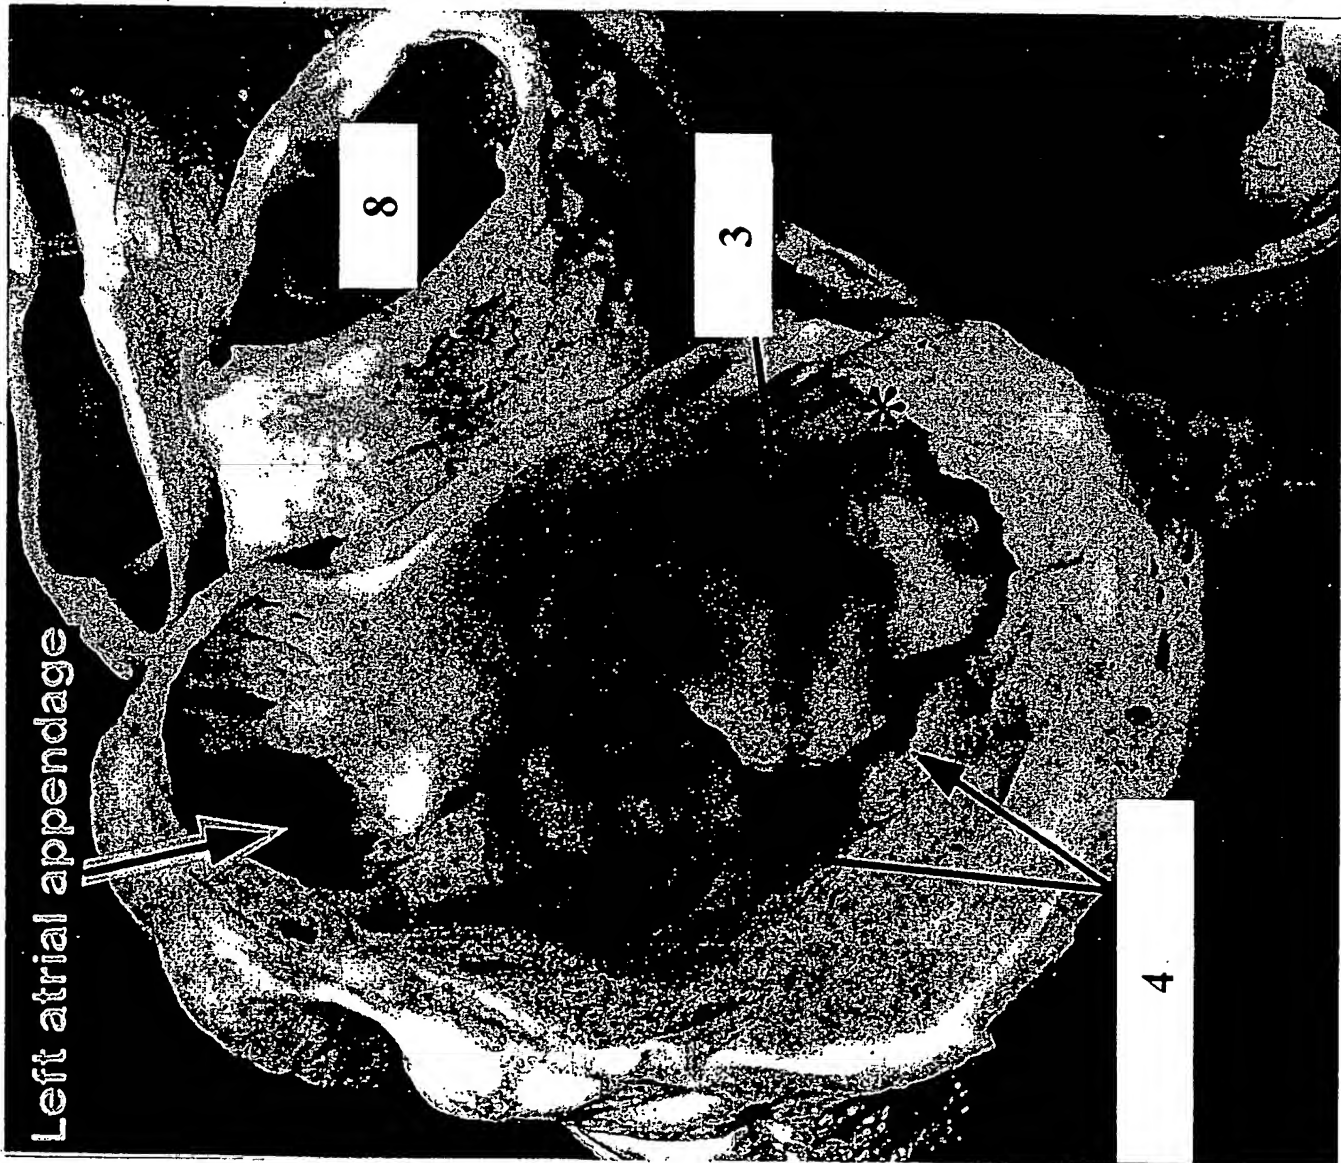


METHODS AND APPARATUS FOR ATRIOVENTRICULAR VALVE REPAIR


Neal L. Eigler et al.

Appl. No.: 10/628,880 Atty Docket: CEDAR.001A

Replacement Sheet  
Reply to Office Action  
of June 15, 2006

Best Available Copy

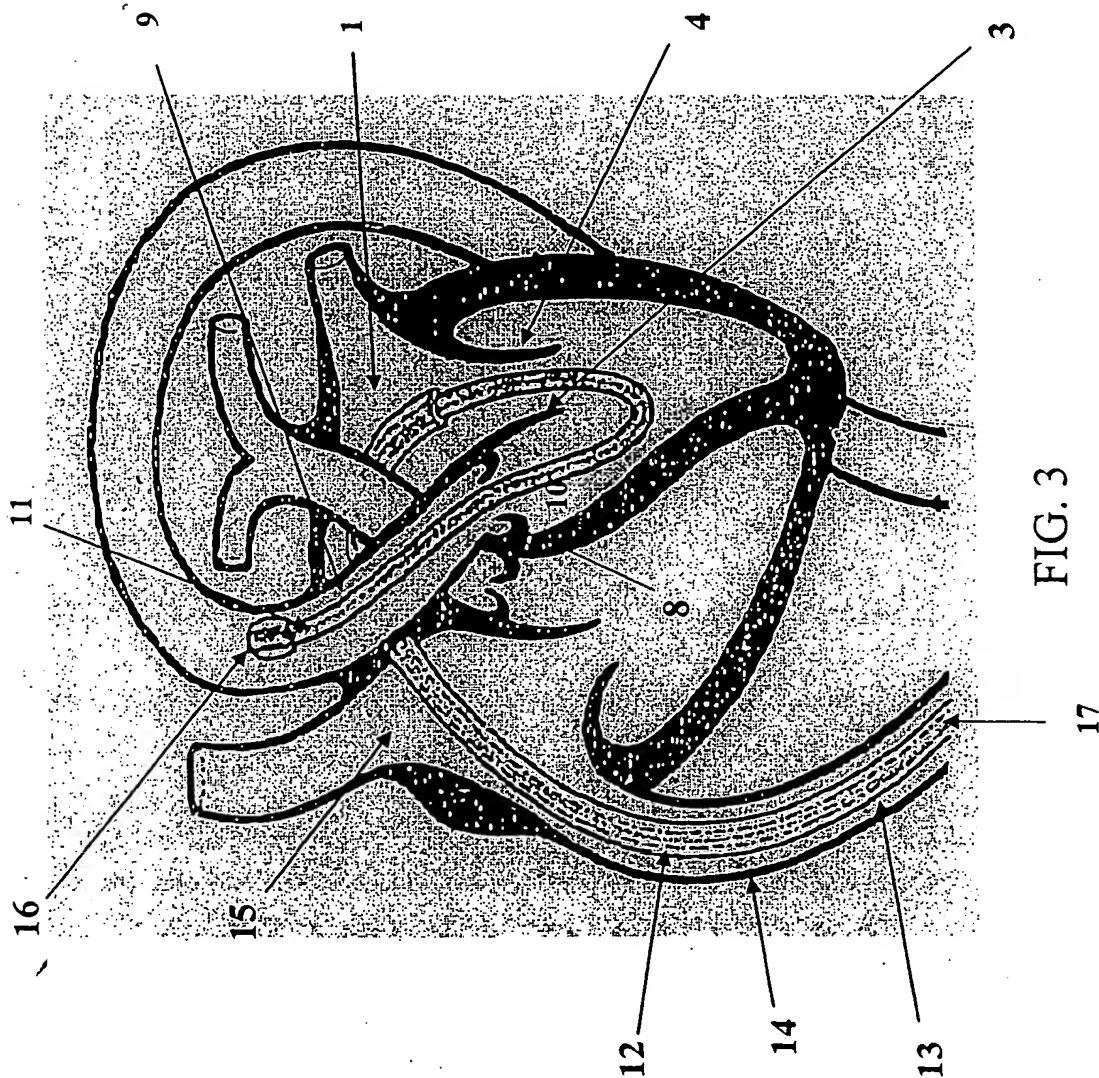

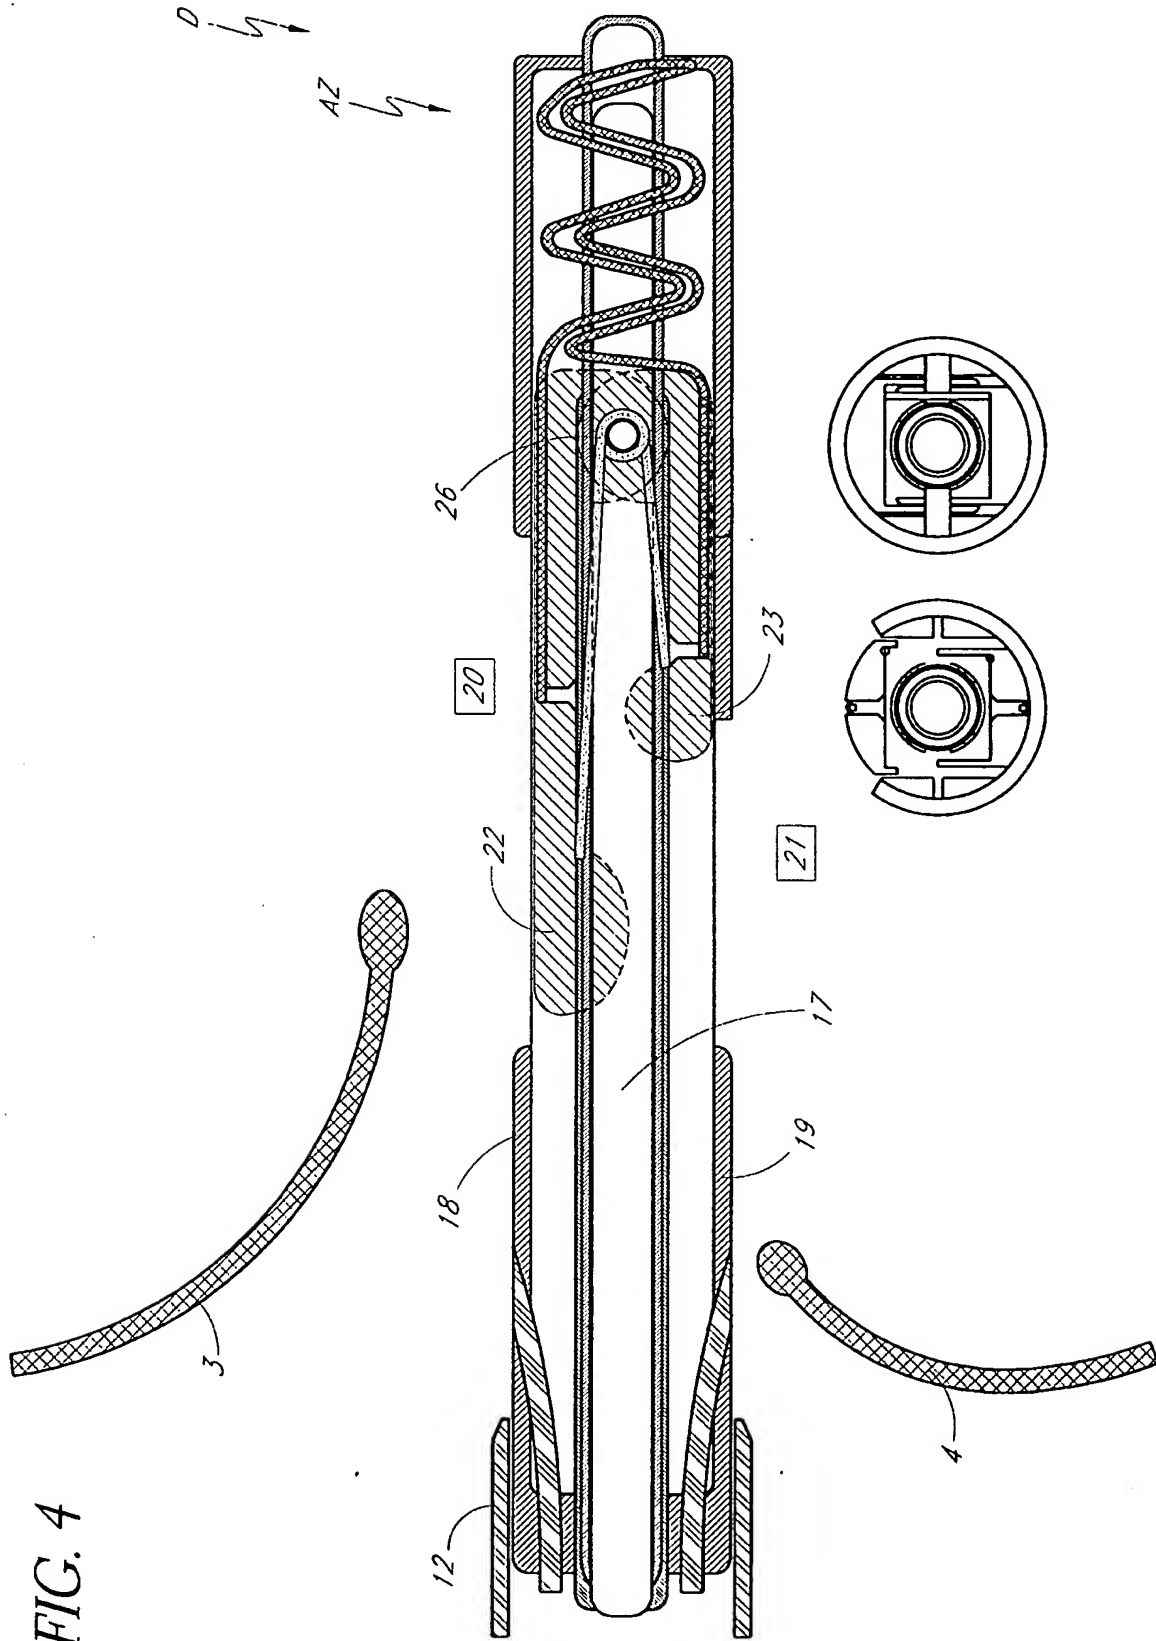


**FIG. 5**

METHODS AND APPARATUS FOR ATRIOVENTRICULAR VALVE REPAIR

Neal L. Eigler et al.

Appl. No.: 10/628,880 Atty Docket: CEDAR.001A

Replacement Sheet  
Reply to Office Action  
of June 15, 2006

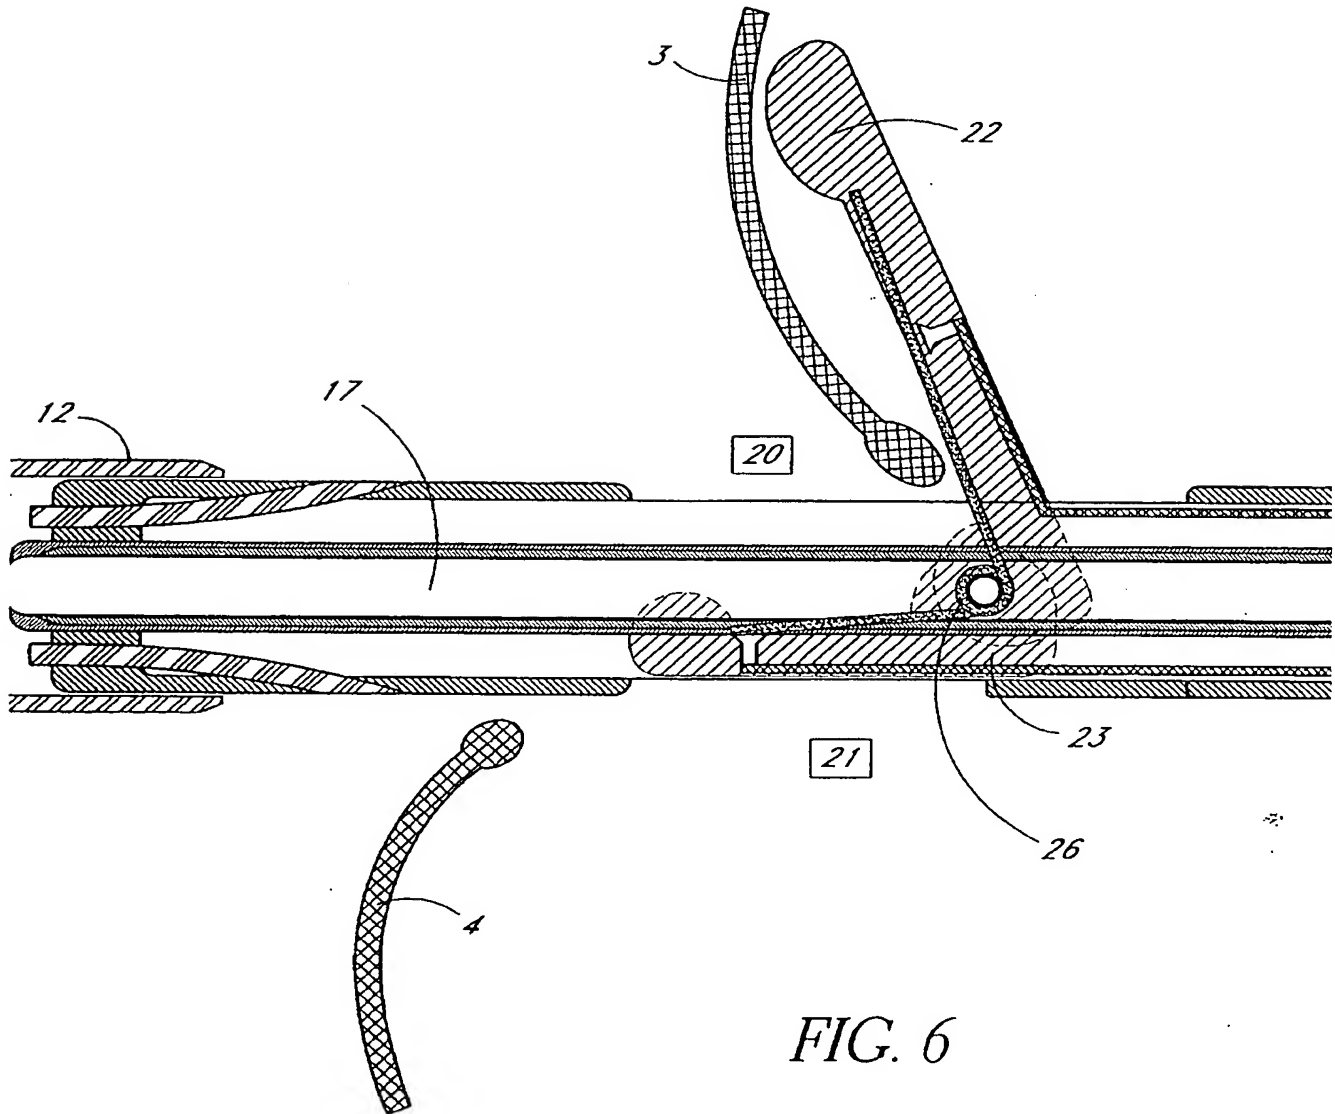

METHODS AND APPARATUS FOR ATRIOVENTRICULAR VALVE REPAIR

Replacement Sheet  
Reply to Office Action  
of June 15, 2006

Neal L. Eigler et al.  
Appl. No.: 10/628,880 Atty Docket: CEDAR.001A


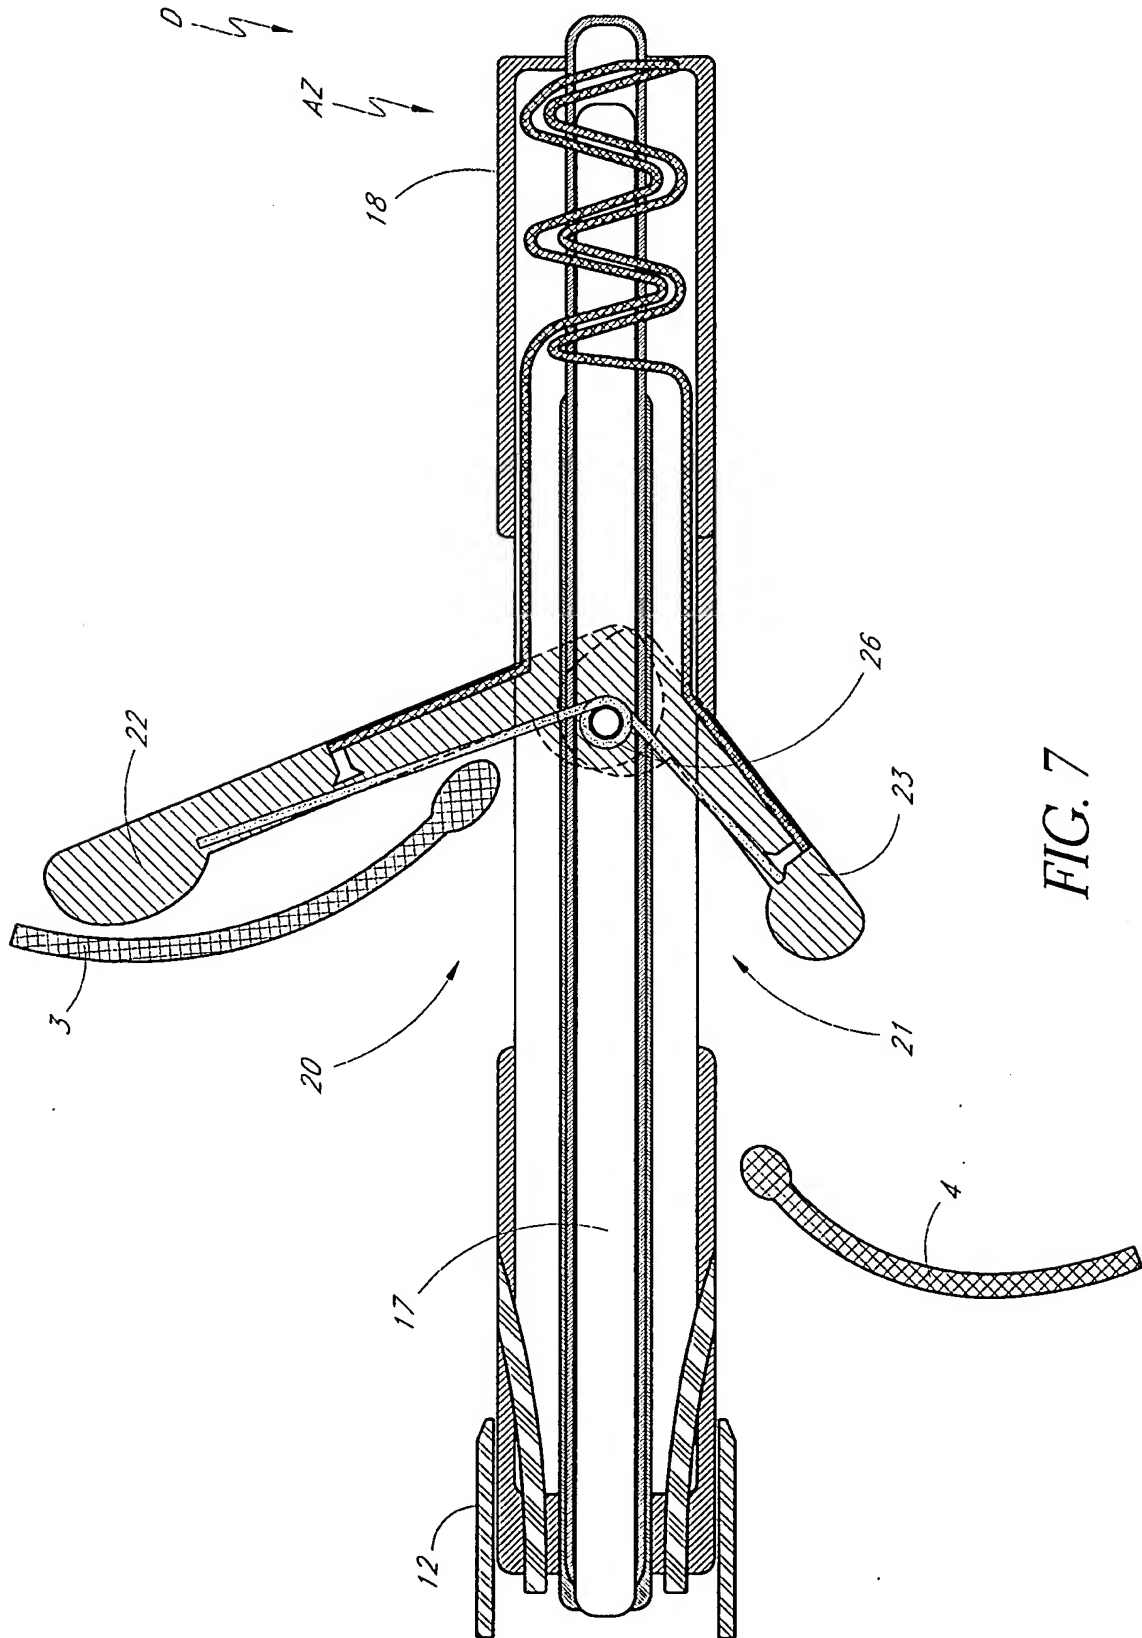


FIG. 7

METHODS AND APPARATUS FOR ATRIOVENTRICULAR VALVE REPAIR

Replacement Sheet  
Reply to Office Action  
of June 15, 2006

Neal L. Eigler et al.  
Appl. No.: 10/628,880 Atty Docket: CEDAR.001A

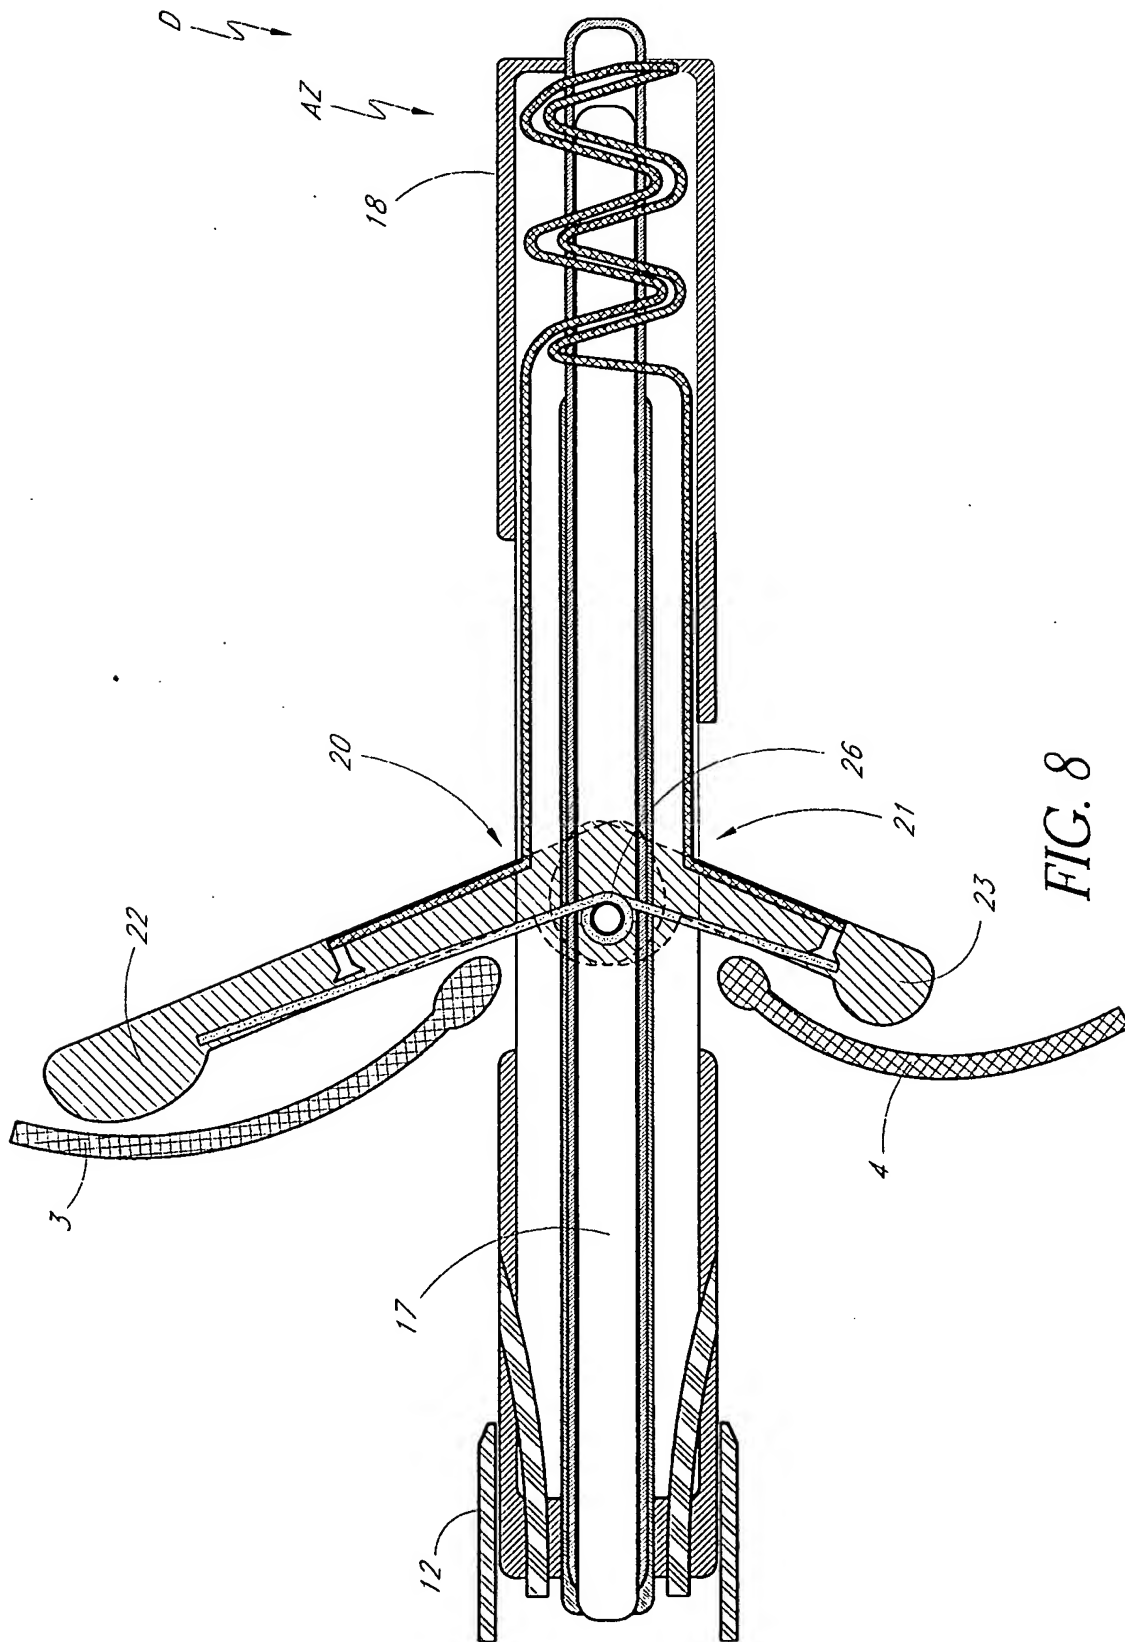



## Neal L. Eigler et al.


*Appl. No.: 10/628,880 Atty Docket: CEDAR.001A*



METHODS AND APPARATUS FOR ATRIOVENTRICULAR VALVE REPAIR

Replacement Sheet  
Reply to Office Action  
of June 15, 2006

Neal L. Eigler et al.  
Appl. No.: 10/628,880 Atty Docket: CEDAR.001A

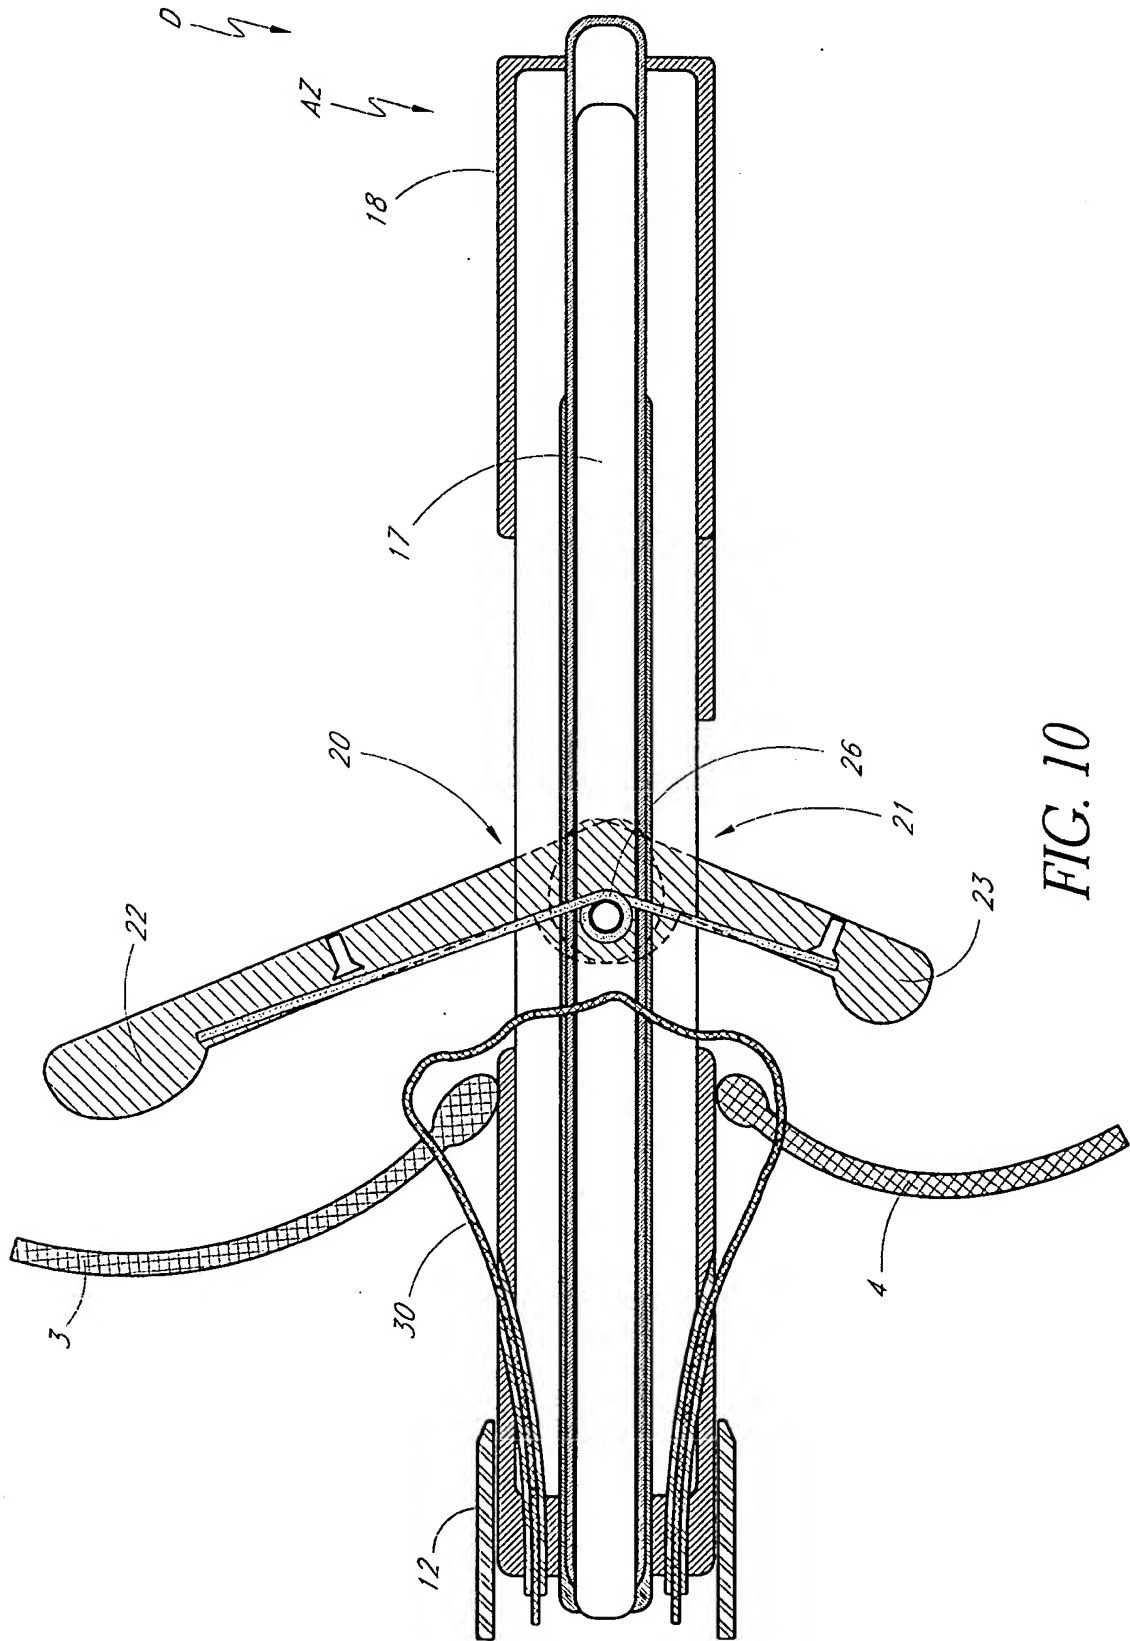

*Replacement Sheet  
Reply to Office Action  
of June 15, 2006*

*Appl. No.: 10/628,880 Atty Docket: CEDAR.001A*

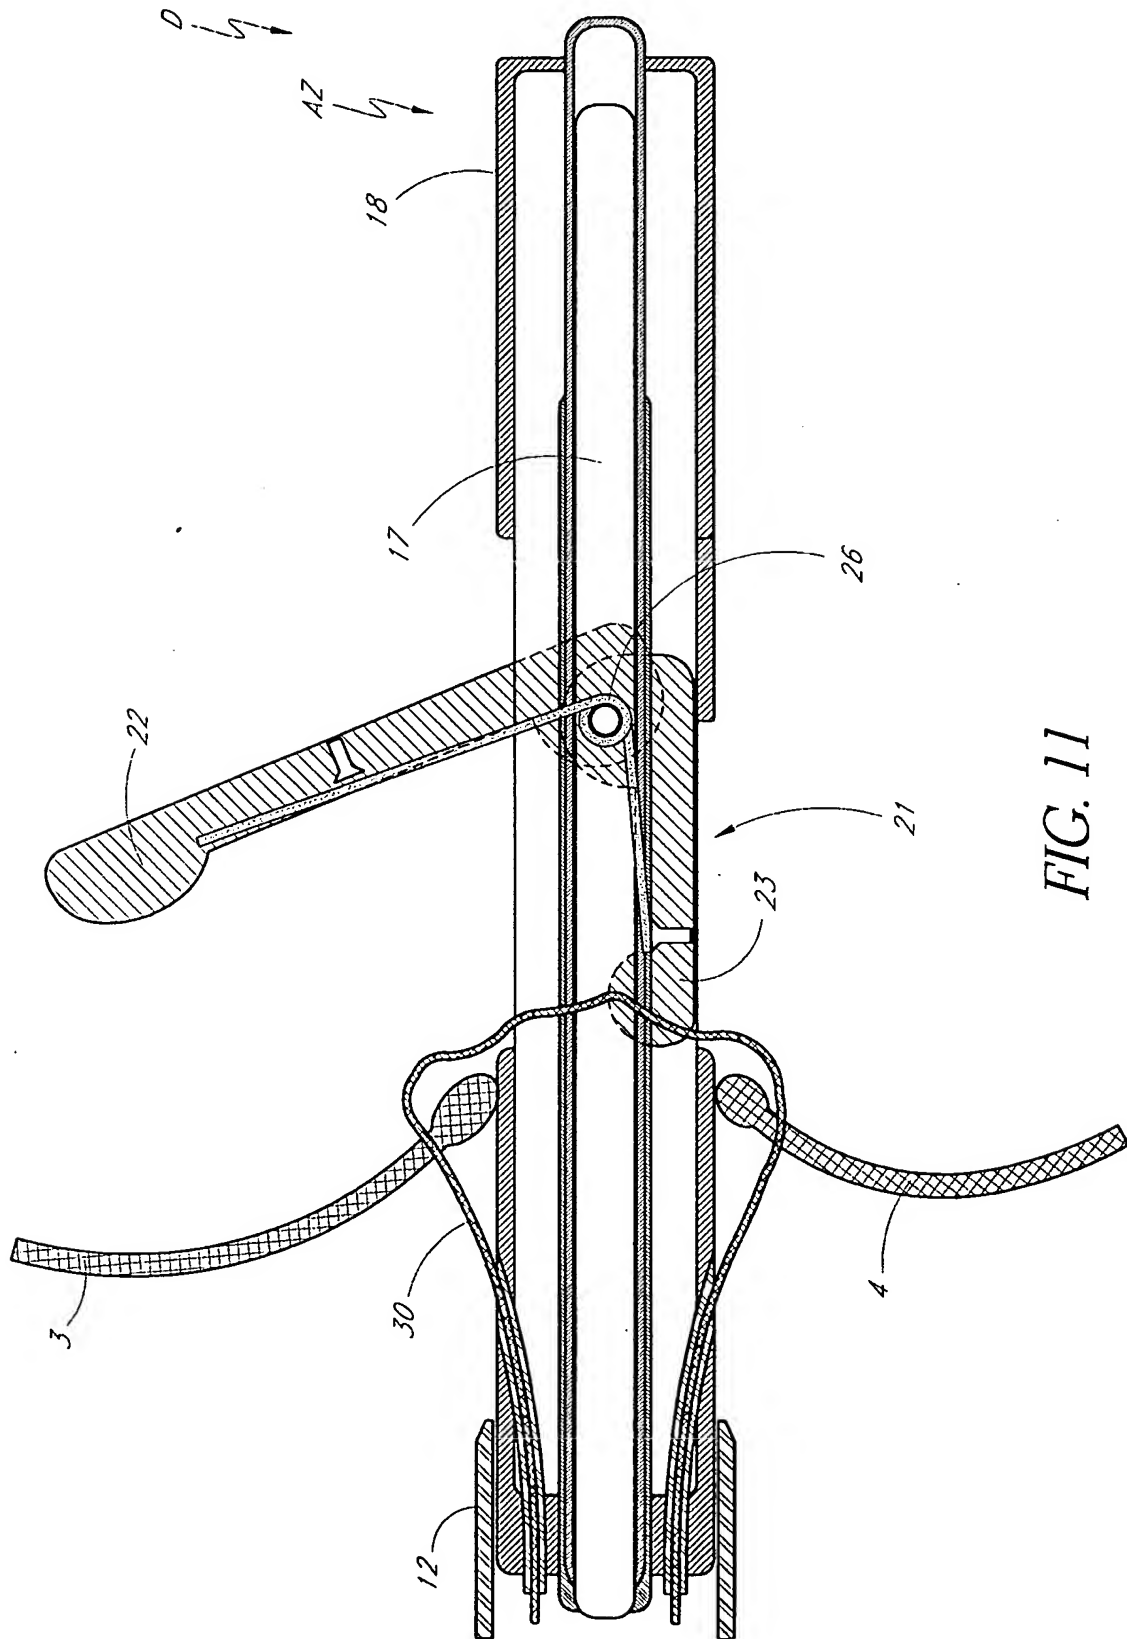


FIG. 11

METHODS AND APPARATUS FOR ATRIOVENTRICULAR VALVE REPAIR

Replacement Sheet  
Reply to Office Action  
of June 15, 2006

Neal L. Eigler et al.  
Appl. No.: 10/628,880 Atty Docket: CEDAR.001A

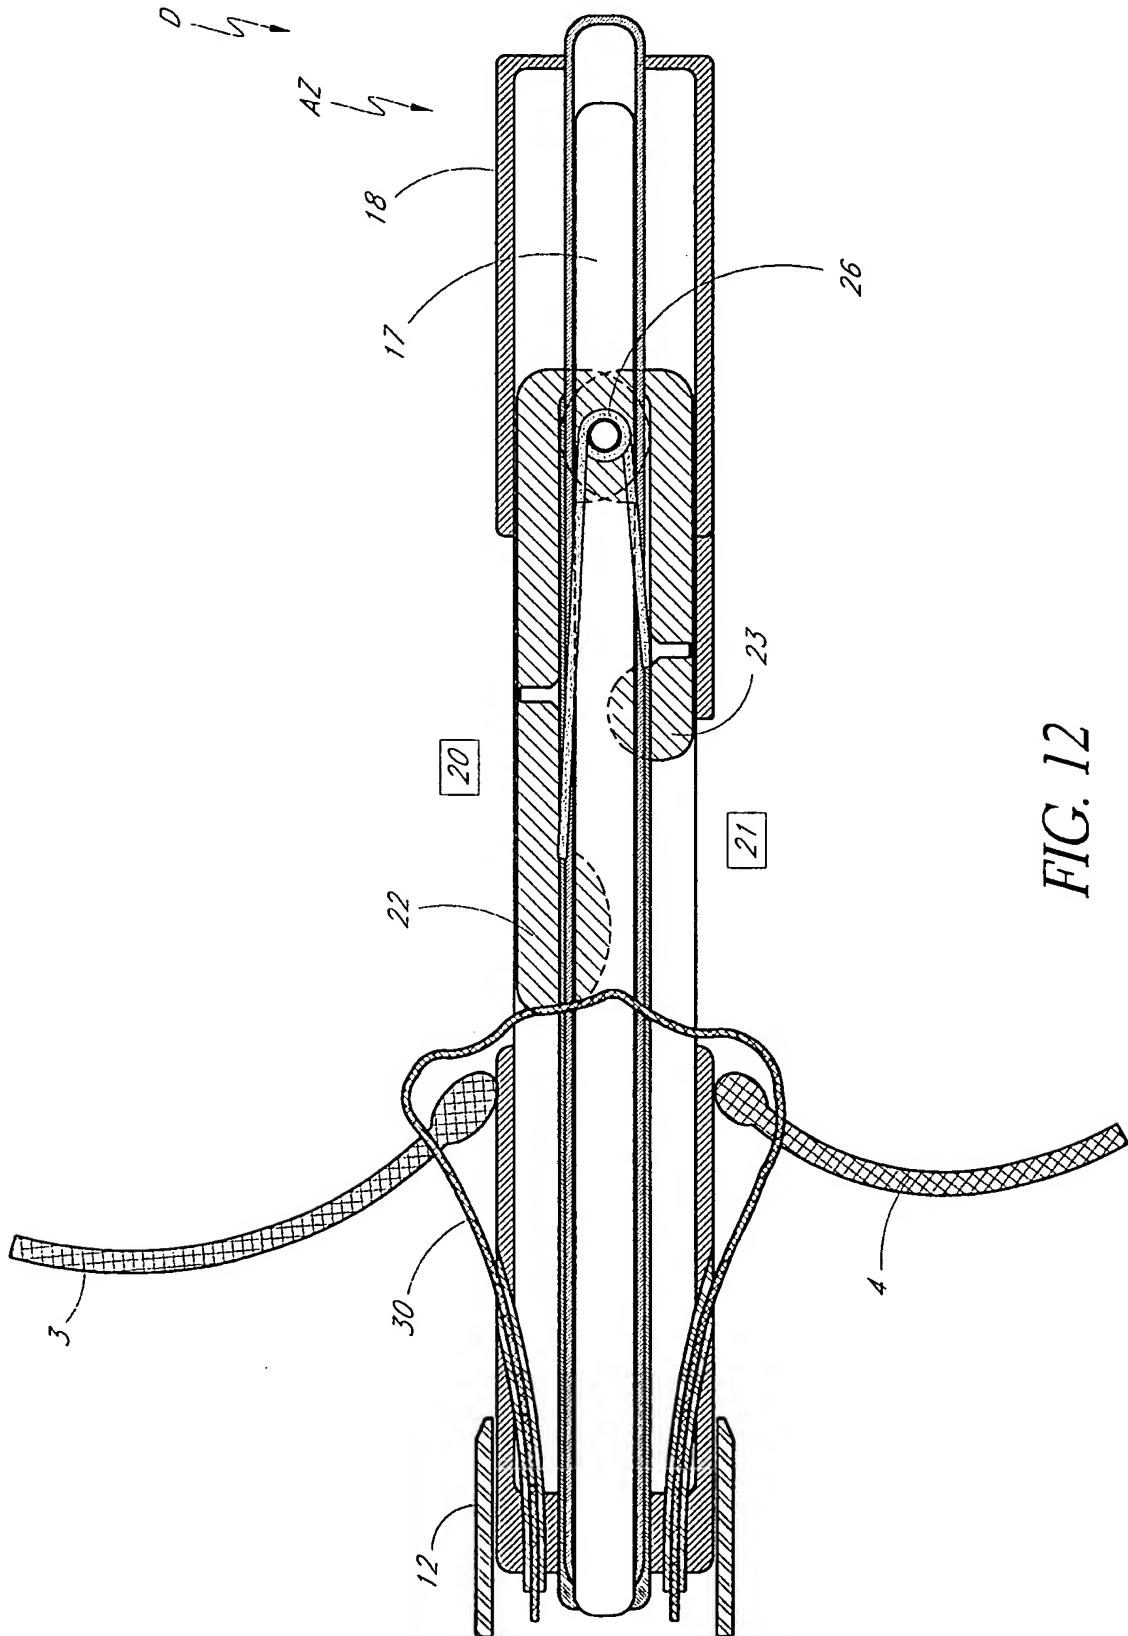


FIG. 12


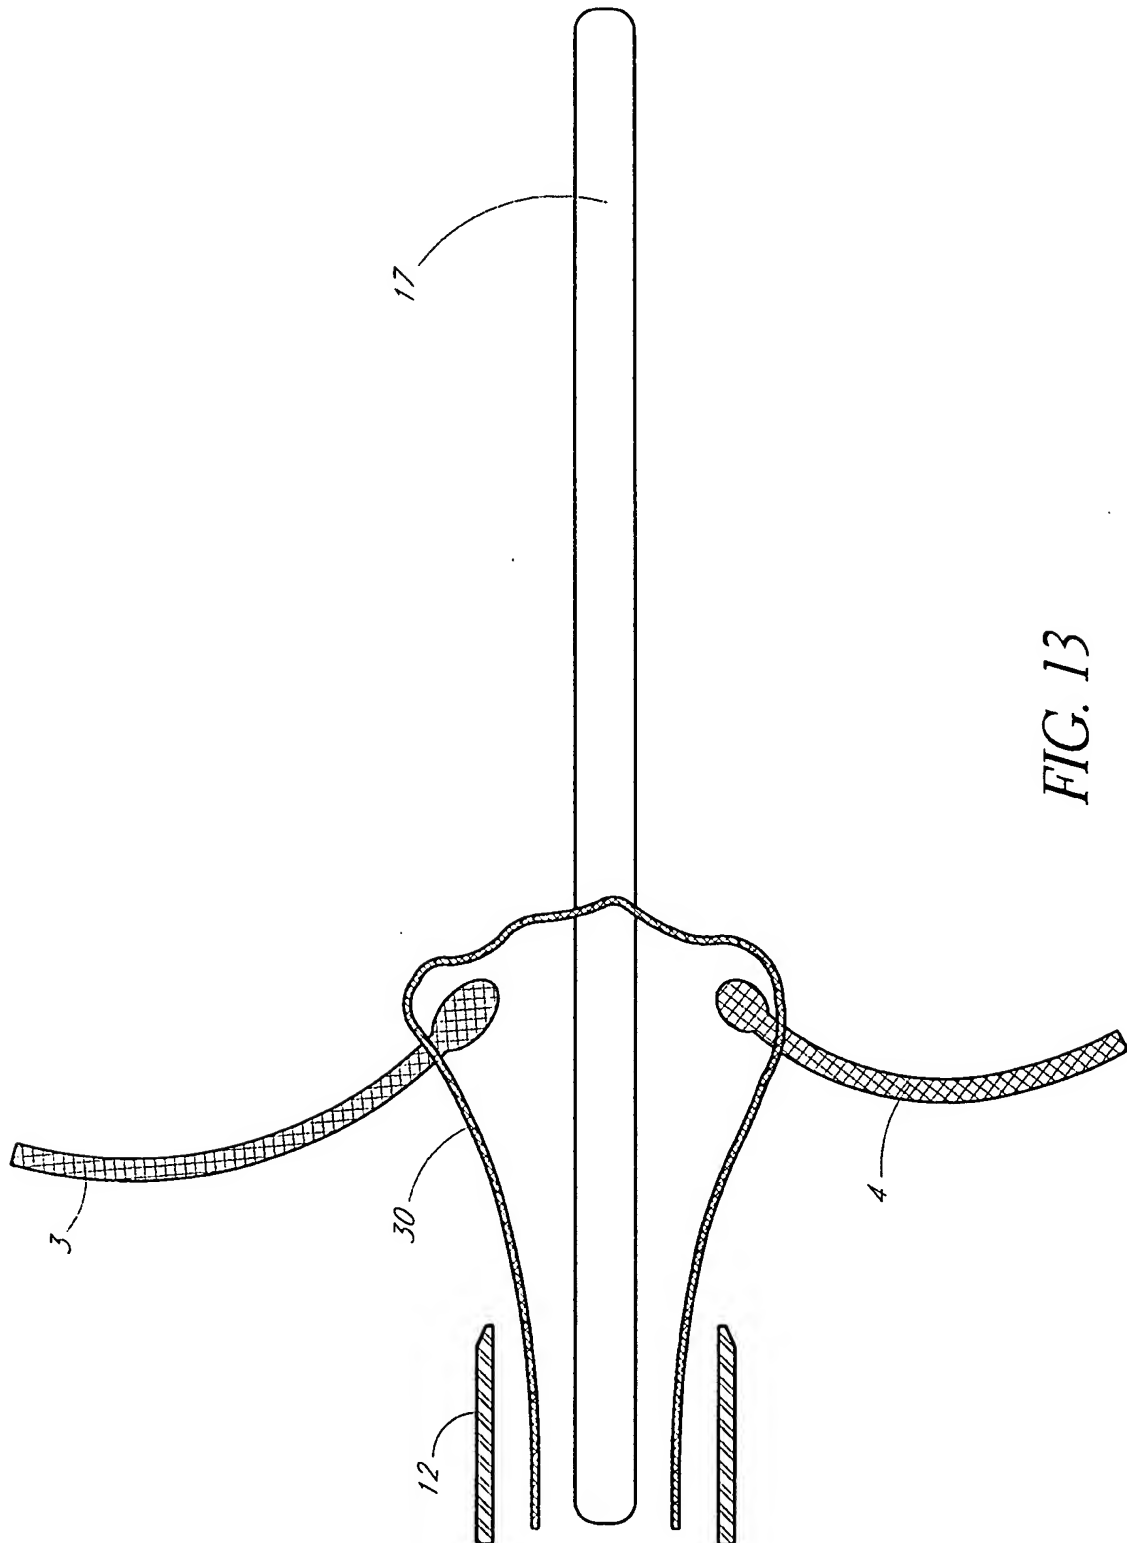


FIG. 13

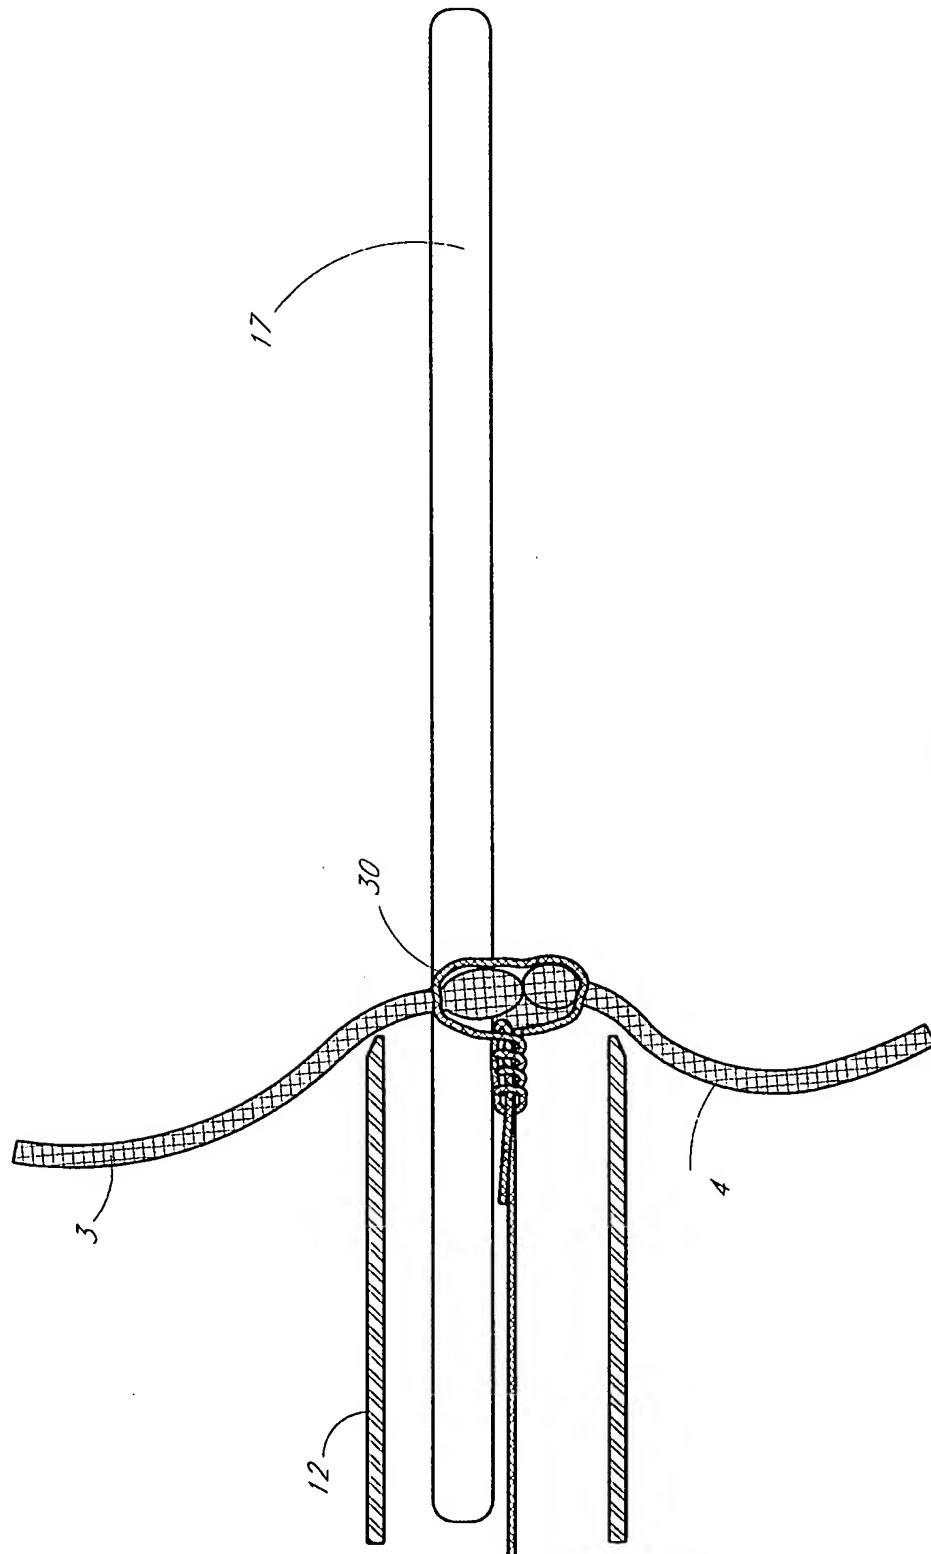

METHODS AND APPARATUS FOR ATRIOVENTRICULAR VALVE REPAIR

Replacement Sheet  
Reply to Office Action  
of June 15, 2006

Neal L. Eigler et al.

Appl. No.: 10/628,880 Atty Docket: CEDAR.001A

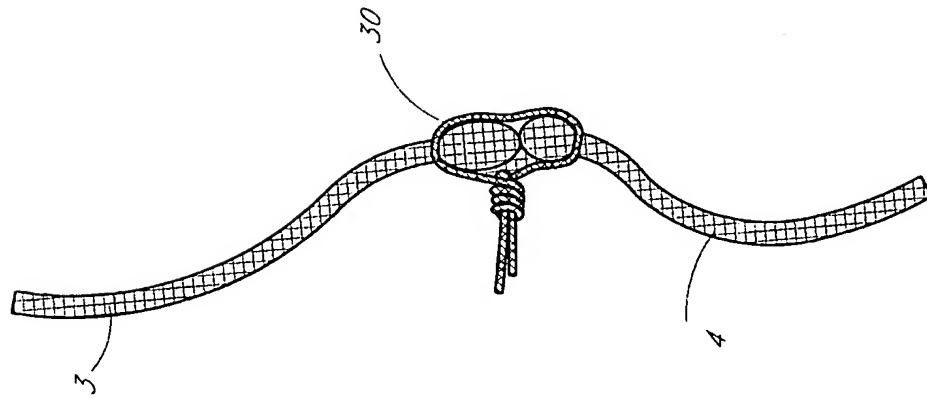


FIG. 15

